

ISOMAG ™

The friendly magmeter

ML210

HIGH PERFORMANCE CONVERTER



GRAPHIC DISPLAY CONVERTER

Warranty conditions are available on this website:
www.isomag.eu only in English version


ISOIL 
INDUSTRIA
The solutions that count

TECHNICAL DATA


Suitable For	<ul style="list-style-type: none"> All the ISOMAG sensors (Ex excluded)
Minimum Conductivity	<ul style="list-style-type: none"> 5 μS/cm
Housing Materials	<ul style="list-style-type: none"> Wall/Compact: Painted Aluminium die casting (OPT. AISI304)
Dimensions	<ul style="list-style-type: none"> See Drawing
Protection Rate	<ul style="list-style-type: none"> IP 67 / IP 68 (OPTIONAL)
Conn. Sensor Cable/Cable Gland	<ul style="list-style-type: none"> CABLE C015 - C016 / N° 6 CABLE GLAND PG 11
Ambient Temperature	<ul style="list-style-type: none"> -20... +60°C / -4... +140 °F
Lcd Display	<ul style="list-style-type: none"> Graphic display 128x64 pixels with back light
Keyboard	<ul style="list-style-type: none"> 3 membrane keys
Pulses/Frequency Outputs	<ul style="list-style-type: none"> N°2 , 1250 Hz, 100mA, 40 Vdc (12,5 KHz Opt.)
Current Output	<ul style="list-style-type: none"> N°1 , 0/4...20mA – RL=1000Ω (+1 Opt.)
Dig. Input / Alarm Output	<ul style="list-style-type: none"> Programmable function
Data Logger	<ul style="list-style-type: none"> 32 values + 64 alarm events
Bi-Directional	<ul style="list-style-type: none"> Yes
Dual Range	<ul style="list-style-type: none"> Yes
FS Value	<ul style="list-style-type: none"> 0,4...10m/s
Communication Port	<ul style="list-style-type: none"> RS 485 (RS232 Opt.)
Protocols	<ul style="list-style-type: none"> ETP (Standard) - Profibus DP/HART/Modbus (opt.)
Diagnostic Funct.	<ul style="list-style-type: none"> Yes
Empty Pipe Detect.	<ul style="list-style-type: none"> Yes
Galvanic Isolation	<ul style="list-style-type: none"> All the inputs/outputs are galvanically isolated from power supply up to 500 V
Data Storage	<ul style="list-style-type: none"> Eeprom values storing system in case of power failure
Programming Plug In	<ul style="list-style-type: none"> Protected plug in for the connection to PC or hand terminal
Batch Function	<ul style="list-style-type: none"> Yes
CE Certification	<ul style="list-style-type: none"> Yes
Measurements Tolerance	<ul style="list-style-type: none"> Flow rate (volume) = $\pm 0,05\%$ v.l. Out 4/20 mA = $\pm 0,08\%$ v.l. Frequency Out = $\pm 0,08\%$ v.l.
Repeatability	<ul style="list-style-type: none"> Better than $\pm 0,1\%$
Accuracy	<ul style="list-style-type: none"> See table below
Altitude	<ul style="list-style-type: none"> -200 m up to 6000 m (- 656 up to 19680 ft)
Humidity Range	<ul style="list-style-type: none"> 0÷100% (IP 67)
Power Supply/Consumption	<ul style="list-style-type: none"> 90÷265 Vac(25VA) – 45÷66 Hz; 18÷63Vdc/15÷45 Vac-45÷66Hz (23 VA) ; 10÷35 Vdc (21W)

OVERALL DIMENSIONS


COMPACT VERSION

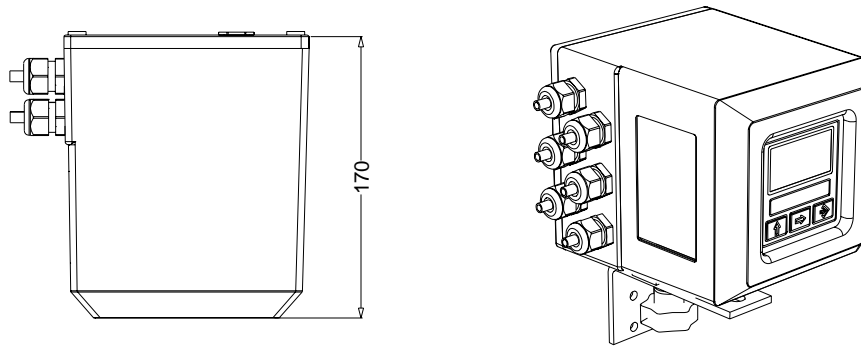


SEPARATE VERSION

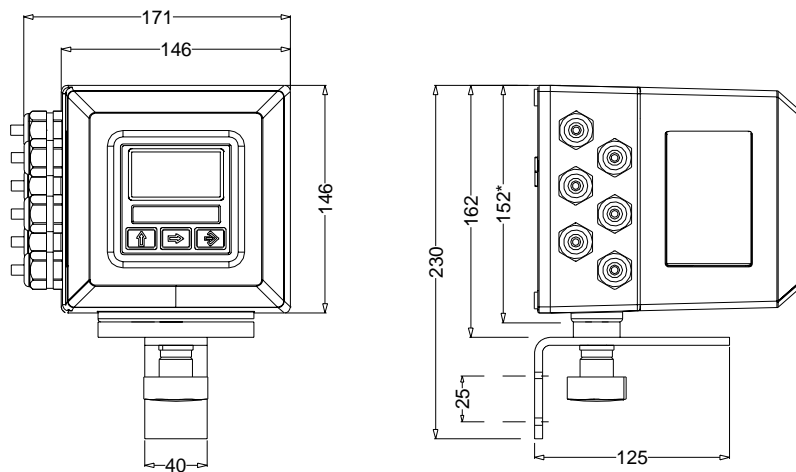


PANEL MOUNTING VERSION

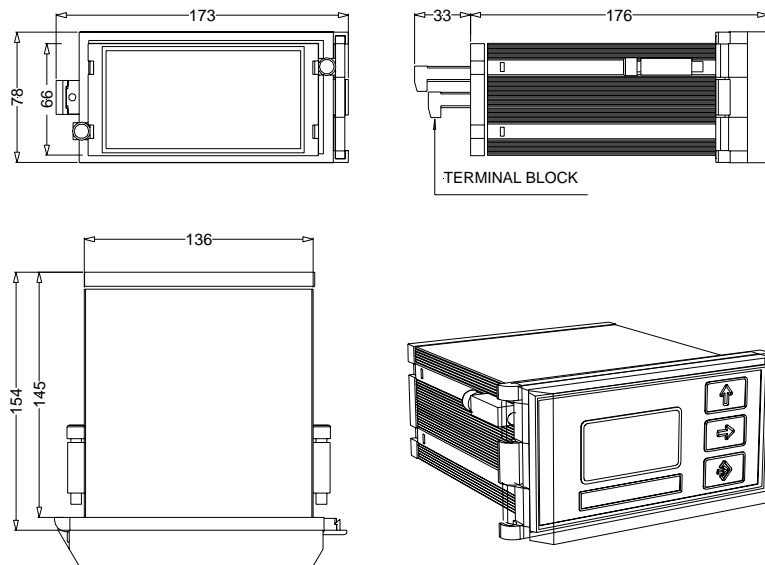

VISUALIZATION PAGES

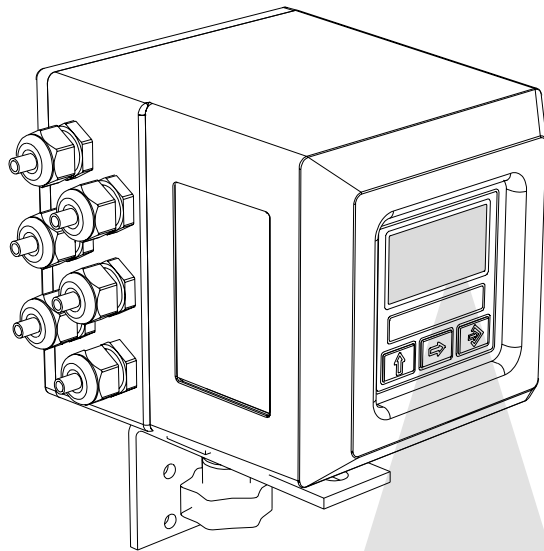


Flowrate and totalizes visualization




Flowrate, speed values and graph



Flowrate value and Full scale % graph



Flowrate graph





Flowrate value with currency function enabled



Different visualisation possibilities with the simple press of a key

ELECTRICAL CONNECTIONS


TERMINAL BLOCK: COMPACT/SEPARATE VERSION

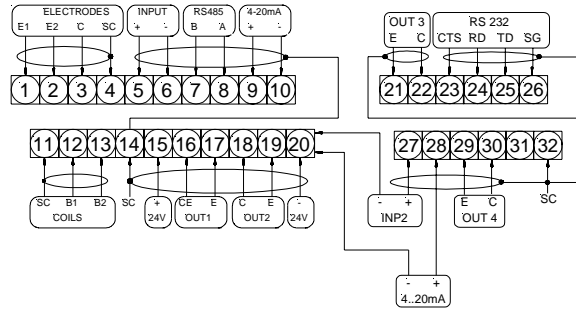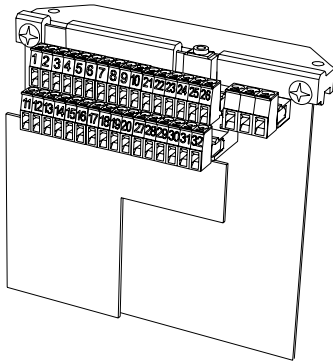

TERMINAL BLOCK: PANEL MOUNTING VERSION

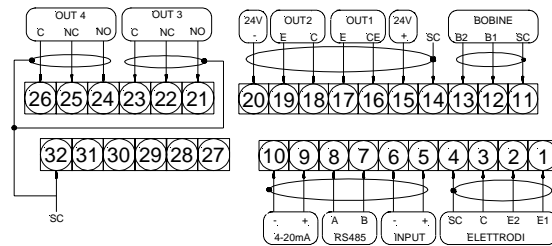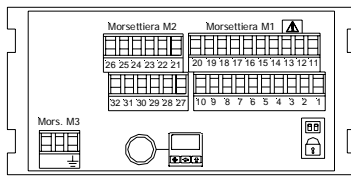


ON/OFF STANDARD OUT





OUT 4/20 mA

ON/OFF HIGH FREQUENCY

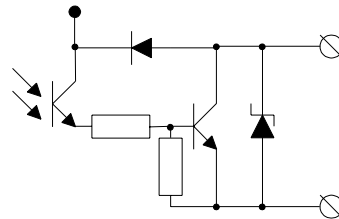

ON/OFF INPUT

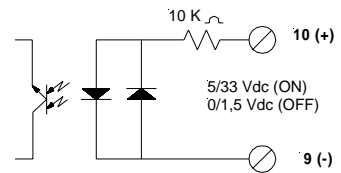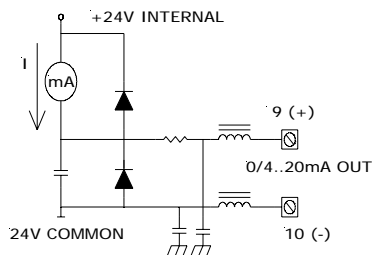

FUNCTIONS

MAIN MENU

1-Sensor

```

1-SENSOR
ND=mm 00032
KA= +01.0080
Sens.type= 000
Ins.position= 0
KL=+101 +02.1500
KR=-101 +02.1500
Cable len.=m 000
E.P.detect= OFF
E.p.thr.= 250
Autozero cal.

```

- .1.1 Insert ND of sensor (0-3000mm)
- .1.2 Sensor calibration data, visualized on sensor's label
- .1.3 Type of sensor: Enter the first two characters of the serial number of the sensor
- .1.4 Position for insertion sensors: 0=1/8DN, 1=1/2DN, 2=7/8DN
- .1.5 Factory parameters
- .1.6 Length of the cable connecting the sensor to the converter
- .1.7 Enables the empty pipe detection feature
- .1.8 Value of empty pipe sensibility detection
- .1.9* Enables the automatic zero calibration system

MAIN MENU

1-Sensor

2-Scales

```

2-SCALES
Fs1=dm³/s 5.0000
Fs2=dm³/s 8.1920
Tot.MU=dm³ 1.000
Pls1=dm³ 1.00000
Pls2=dm³ 1.00000
Tpls1=ms 0050.00
Tpls2=ms 0050.00
Frg1=Hz 1000.00
Frg2=Hz 1000.00
Mass units= ON
Sg=kg/dm³ 01.0000

```

- .2.1* Full scale value set for range N.1
- .2.2* Full scale value set for range N.2
- .2.3* Unit of measure and number of decimal totalizes
- .2.4* Pulse value on channel 1
- .2.5* Pulse value on channel 2
- .2.6* Duration of the pulse generated on channel 1
- .2.7* Duration of the pulse generated on channel 2
- .2.8 Full scale freq. for channel 1 (0.1Hz-1000.0Hz) (0.1Hz-10000Hz con modulo opt.)
- .2.9 Full scale freq. for channel 2 (0.1Hz-1000.0Hz) (0.1Hz-10000Hz con modulo opt.)
- .2.10 Enable/disable the selection of mass units on full scale set
- .2.11 Specific gravity set in kg/dm³

MAIN MENU

1-Sensor

2-Scales

3-Measure

```

3-MEASURE
Iconst=s 0001.0
Filter=s 0.1
Skip thr=% 010
Peak thr=% 125
Cut-off=% 05.0
Autocal.= OFF
Autorange= OFF
E.saving= OFF

```

- .3.1* Time constant
- .3.2 Filter on the power supply: 0.1s="ready" measure; 0.5s=filter of noise on the liquid
- .3.3* Acceleration threshold
- .3.4* Anomalous signal pick cut off threshold
- .3.5 Low flow zero threshold: 0-25% of full scale value
- .3.6 Enable every hour an internal cycle of calibration. Measurement stopped for 8-15 sec.
- .3.7* Automatic change of scale
- .3.8* Energy saving mode

MAIN MENU

1-Sensor

2-Scales

3-Measure

4-ALARMS

```

4-ALARMS
Max thr+=% 000
Max thr-=% 000
Min thr+=% 000
Min thr-=% 000
Hyst.=% 03
E.p.thr.= 075
mA v.fault=% 000
Hz v.fault=% 125
Timeout=s 00.0

```

- .4.1 Maximum value alarm set for direct flow rate
- .4.2 Maximum value alarm set for reverse flow rate
- .4.3 Minimum value alarm set for direct flow rate
- .4.4 Minimum value alarm set for reverse flow rate
- .4.5 Hysteresis threshold set for the minimum and maximum flow rate alarms
- .4.6 Empty pipe detection threshold. It's automatically set by the function 1.9
- .4.7* Current output value in case of failure
- .4.8* Frequency output value in case of failure
- .4.9* Batch safety timer

MAIN MENU

1-Sensor

2-Scales

3-Measure

4-ALARMS

5-INPUTS

```

5-INPUTS
I+ RESET= ON
P+ RESET= ON
I- RESET= OFF
P- RESET= ON
Puls.reset= OFF
Count lock= ON
Calibration= OFF
Range change= OFF
Batch= OFF
Inp.2= OFF

```

- .5.1* Total direct (positive) flow totalise reset enable
- .5.2* Partial direct (positive) flow totalise reset enable
- .5.3* Total reverse (negative) flow totalise reset enable
- .5.4* Partial reverse (negative) flow totalise reset enable
- .5.5 Reset totalise of pulse from digital input (see page 15)
- .5.6 Totalise counting lock command (see page 15)
- .5.7* Autozero calibration external command
- .5.8 Range change external command (vedi funzione 3.7)
- .5.9 Batch start/stop external command (see batch functions)
- .5.10* Functions assigned to input 2

MAIN MENU

1-Sensor

2-Scales

3-Measure

4-ALARMS

5-INPUTS

6-OUTPUTS

```

6-OUTPUTS
Out1= #1 IMP+
Out2= SIGN
Out3= OFF
Out4= #2 IMP+
Duty cycle1=% 50
Out mA1=4÷22
Out mA2=4÷22

```

- .6.1* Output 1 functions
- .6.2* Output 2 functions
- .6.3* Output 3 functions
- .6.4* Output 4 functions
- .6.5* Duty cycle value for pulses/frequency output
- .6.6* Choice of the function and the range of current output n.1
- .6.7* Choice of the function and the range of current output n.2

```

7- COMMUNICATION
IF2 prot.= DPP
RS232 prot.= DPP
Address= 000
RS485 bps= 19200
RS232 bps= 4800
Printer= OFF
Print batch= OFF
Print data= OFF
Print events= OFF
Rem. addr.= 000
Remote u.conn.

```

- 7.1 Choice of the communication protocol for the IF2 device
- 7.2 Choice of the communication protocol for the RS232 port
- 7.3 Address value of converter (range 0 - 255)
- 7.4 Speed of the RS485 output (possible choices: 2400, 9600, 19200, 38400 bps)
- 7.5 Speed of the RS232 output (possible choices: 2400, 9600, 19200, 38400 bps)
- 7.6 Print function enable (optional; see manual MI200)
- 7.7 Print of the performed batch
- 7.8 Stampa dei dati ad intervalli regolari ed impostabili
- 7.9 Print of the data process on regular intervals
- 7.10 Address of a further converter connected like a terminal
- 7.11 Start remote connection to the terminal. Connection interrupted after 10sec. of inactivity

```

8-DISPLAY
Language= EN
D.rate=Hz 1
Contrast= 7
P.totaliz.= ON
Date/time= OFF
Quick start= OFF
Tot.modif.= OFF
Net total.= OFF
Reset video= OFF
Currency= ON
Curr.decim.= 2
EUR/dm3+ 1.00000
EUR/dm3- 1.00000

```

- 8.1 Choice of the language: EN= English, IT=italian, FR= French, SP= Spanish
- 8.2 Updating frequency on the display: 1-2-5-10 Hz
- 8.3* Display contrast
- 8.4 Partial totalizer visualization (with batch enable the function is always on)
- 8.5 Date and time visualization with data logger enable
- 8.6 Quick start menu visualization
- 8.7 Enable the change value of the totalises (see function 5.1-5.4)
- 8.8* Enable the page of net totalizer (difference between direct and reverse. see page 22)
- 8.9 Reset the processor of the display (useful in case of particular badly operations of the display)
- 8.10 Visualizes the values of the partial totalise in the unit of selected currency
- 8.11 Choice of the numbers of decimals for the visualization currency value: From 0 to 3
- 8.12*Value of conversion/currency for direct totalizer
- 8.13*Value of conversion/currency for reverse totalizer

```

9-DATA LOGGER
1992/05/10 15:03
Acquisition= ON
Interval-h 24
Display data
Display events
Disp.min/max
Clear data
Clear events
Reset min/max

```

- 9.1* Date and time set
- 9.2 Automatic data logger enable
- 9.3 Interval time for the data logging function: 1, 2, 3, 6, 8, 12, 24, 48 hours
- 9.4 Displaying of the data stored in the data logger
- 9.5 Displaying of the last 64 alarms stored in the data logger
- 9.6 Visualization function of minimum and maximum peak of flow rate
- 9.7 Logged data cancel function
- 9.8 Reset all alarm events
- 9.9 Reset all minimum and maximum peak of flow rate stored

```

10-DIAGNOSTIC
Calibration
Self test
Simulation= OFF

```

- 9.2 Automatic data logger enable
- 9.3 Interval time for the data logging function: 1, 2, 3, 6, 8, 12, 24, 48 hours
- 9.4 Displaying of the data stored in the data logger

```

8-Display
9-Data logger
10-DIAGNOSTIC
11-INTERNAL DATA
12-Batch

```

```

11-INTERNAL DATA
L2 keycode=00000
Lock level= 3
Load fact.pres.
Load user pres.
Save user pres.
Hours= 0000??
Ign.cal.err= OFF
KS= +1.0000

```

- 11.1 Level 2 access code enter
- 11.2 Block level function can be set from 0 to 3
- 11.3 Load factory data pre-set
- 11.4 Load user data saved
- 11.5 Save user data
- 11.6 Visualisation of the total operation hours of the converter (function not editable)
- 11.7 Ignore the calibration error during the switch on test
- 11.8 Ks Coefficient

Menu 12: Menu visualized only with batch active

```

12-BATCH
N.samples= 000
Diff.thr=% 010
U.com=dm 00.000
U.pre=dm 00.000
Auto batch= OFF
BM auto sel= OFF
Cons.mode= OFF

```


- 12.1* Number of batch cycles to define the value of compensation. Value 0=OFF
- 12.2* % limit of compensation threshold
- 12.3* Compensation value
- 12.4* Prebatch value
- 12.5* Auto-batch
- 12.6* Automatic selection of batch formula
- 12.7* Static consent of batch

```

8-Display
9-Data logger
10-DIAGNOSTIC
11-INTERNAL DATA
12-Batch

```

ACCURACY TABLE

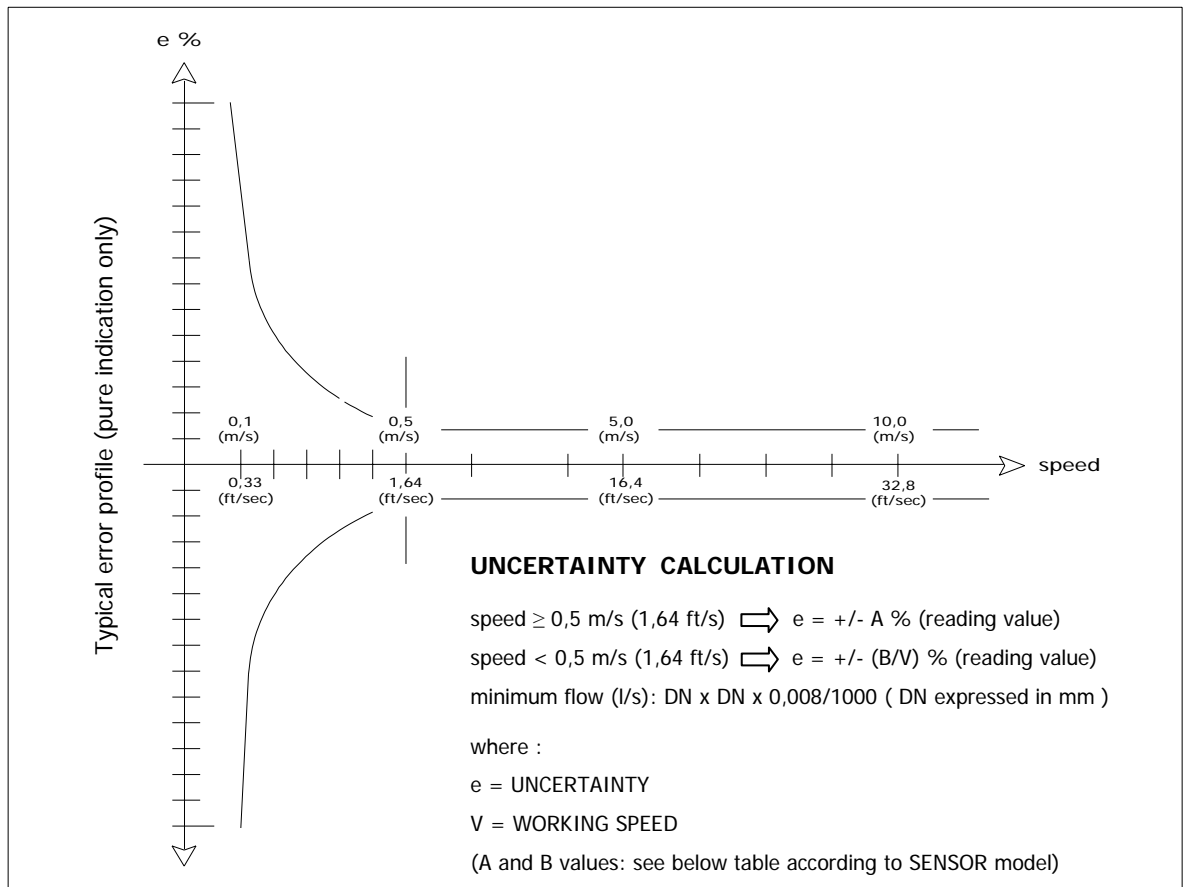

FULL BORE SENSORS

MS501/MS1000/MS2410/MS2500			MS 600			MS5000		
A	B(m/s)	B(ft/s)	A	B(m/s)	B(ft/s)	A	B(m/s)	B(ft/s)
0,2	0,1	0,33	0,4	0,2	0,66	2	1	3,28

INSERTION SENSORS

MS3770			MS3800		
A	B(m/s)	B(ft/s)	A	B(m/s)	B(ft/s)
2	1	3,28	2	1	3,28


Reference conditions :

- Constant flow rate during the test
- Pressure: >30 Kpa
- Flow condition : fully developed flow profile
- Zero stability +/- 0,005 %

HOW TO ORDER

ML 210	Display
A	Blind version without display and keyboard
B	Graphic LCD WSTN back light display execution, point matrix 128 x 64, 8 line each of 16 characters and 3 programming keys
Housing material - Protection rate	
0	Painted aluminum die casting (painted RAL6028) ,protection rate IP67
1	Aisi 304 Electro-polish
2	NORYL UL 94 V-0 black (ONLY "F" VERSION) IP 54
3	NORYL UL 94 V-0 BLACK (ONLY "F" VERSION)+TRANSPARENT FRONTAL COVER IP 65
4	Painted aluminum die casting , protection rate IPXX , presett for CUSTOMER CABLE GLAND (Total Dim. Max available 105 x 52 mm)
Version	
A	Compact version with sensor MS.... (liquid maximum temperature 100 °C)
B	Separate version for wall monting, complete with mounting accessories in Carbon Steel (painted RAL6028)
D	Separate version (CABLE C015-C016 OR C014 with preamp.) for wall monting, complete with mounting accessories in AISI304
F	Separate version (CABLE C015-C016 OR C014 with preamp.) for FRONT PANEL mounting according DIN 43700(72x144) complete with mounting accessories; AVAILABLE ONLY FOR HOUSING MATERIALS OPTIONS 2 AND 3 (SEE ABOVE)
Power supply	
1	Power supply : 90 ... 265 V 45/66 Hz
2	Power supply : 18...63 V dc / 15...45 V ac - 45...66 Hz
3	Power supply : 10 ... 35 V dc
9	Power supply : other
Analogue output	
A	Without Analogue output 0/4...20/22 mA
B	Analogue output 0/4...20/22 mA
Serial Interface	
1	Without Serial Interface
2	RS485 Serial Interface
3	Modbus protocol over RS485 Serial Interface
Additional module	
A	Without additional module
C	ME200; n. 2 additional ON / OFF programmable output
D	ME201; n. 2 additional ON / OFF programmable output (one of them at 10 KHz frequency)
E	ME202; additional 0/4...20 mA + n.2 ON / OFF programmable output
F	ME203; n. 1 RS232 serial interface + n.2 additional ON / OFF programmable output , 2A - 60 Vca, 60W 125 VA)
G	ME204; n. 1 RS232 serial interface + additional 0/4...20 mA + n.2 ON / OFF program. output Vca, 60W 125 VA)
P	ME205; n. 2 relè output (each with 1 NO contact + 1 NC contact, 2A - 60 Vca, 60W 125 VA)
T	ME207; n. 2 relè output (each with 1 NO contact + 1 NC contact, 2A - 250 Vca, 60W 125 VA)
H	ME 100 : Profibus DP module
M	ME 220 : d. logger r. t. c. ; 128K record : F.R. ;tot.+/-; date/time)
N	ME 221 : d. logger r. t. c. ; 128 Krecord : F.R.;tot.+/-; date/time ; n° 1 RS 232
O	ME 222 : d. logger r. t. c. ; 128K record : F.R.;tot.+/-; date/time ; n° 1 RS 232 , n° 1 RS 485+1 A.I.
Q	ME 200 + ME 220
R	ME 201 + ME 220
S	ME 202 + ME 220
U	ME 203 + ME 220
V	ME 204 + ME 220
B	ME 206 + ME 220
K	ME 207 + ME 220
X	ME 200 + ME 221
Y	ME 201 + ME 221
W	ME 202 + ME 221
L	HART PROTOCOL OUT
Z	Other
Special Features	
0	ANY
1	WITH ANTICONDENSE CAP

ML 210 B 0 A 1 B 2 A 0 CODE EXAMPLE FOR ORDER

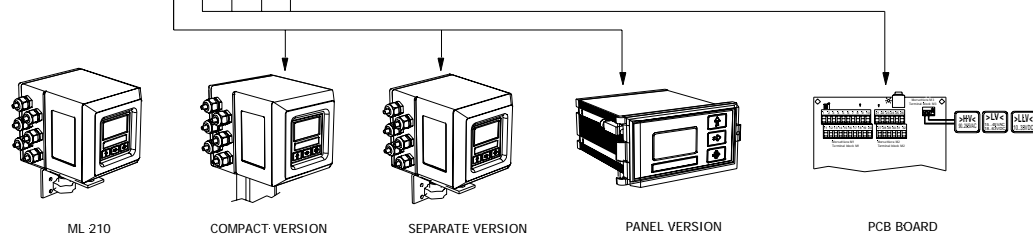

The manufacturer reserves the right to make design improvements without notice.